
OBTURATION SYSTEM. ____ PRODUCTDIAGRAM.





OBTURATION SYSTEM. CLEANING INSTRUCTIONS.

Regular Maintenance (Day to Day Cleaning)


Tools you will need; Multi-Tool • Cleaning brush and Cleaning solution • Disposable cloth (napkin, gauze, etc.)

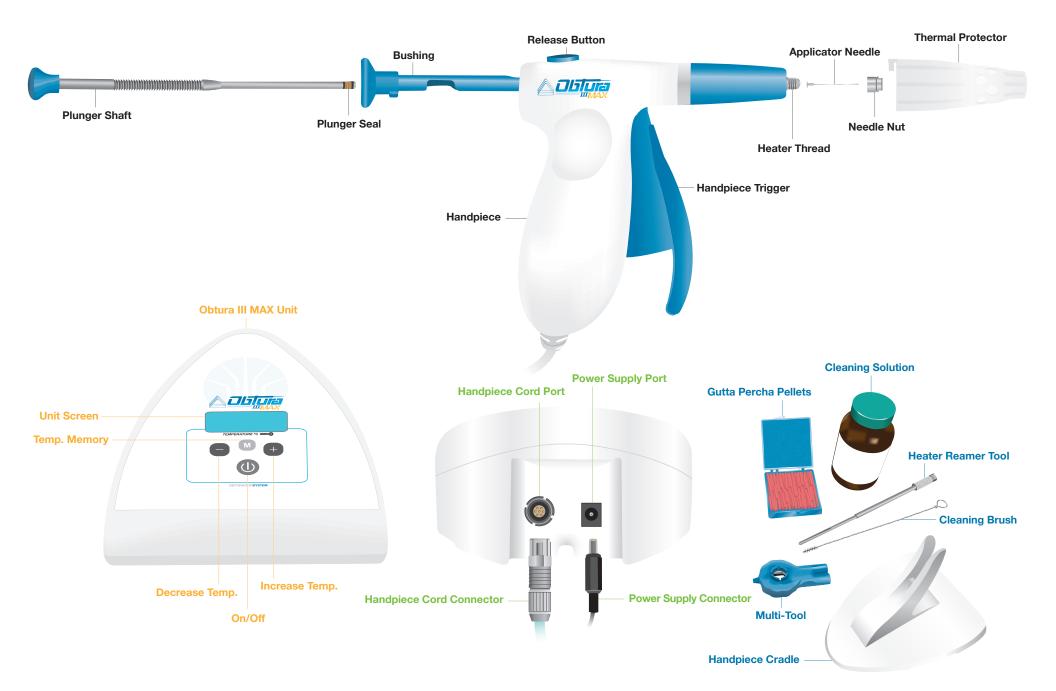





Unlatch and remove the thermal protector using the Multi-Tool.



Use the Multi-Tool to unscrew Set aside the needle nut. Dispose the needle nut from the heater of the needle (for optimum performance, Obtura applicator thread. needles should be used only once).



Extrude all remaining gutta percha by squeezing the handpiece trigger.



Push and hold the release button, removing the plunger shaft from the handpiece.



STEP #6

Inspect the plunger seal for gutta percha.



If gutta percha is present, dip the cleaning brush into the cleaning solution, fully coating gutta percha is cleared.

Clean the plunger seal with the cleaning brush in a back and forth motion until all visible



Inspect the inside of the handpiece shaft for any visible gutta percha.



If gutta percha is present, re-dip Place the cleaning brush inside the cleaning brush into the the handpiece shaft and clean in cleaning solution, fully coating a back and forth motion until all visible gutta percha is cleared.

STEP #8




Reassemble all components in Place the handpiece back on its the reverse order from which cradle.

the brush.



At no point should any part of the Obtura III MAX handpiece be submerged into the cleaning solution.



the brush.

For optimal care, use Birex® solution to clean, disinfect and deodorize your Obtura III MAX unit.

Always spray cleaning solution into a disposable cloth, then wipe down. Never spray directly onto the unit.

they were detached.