


Patient chair swivel

Foot switch

- Press **Release the locking mechanism**
- Keep pressed **Rotate the seat in either direction**
- Release **Lock the seat in one of the locking positions**



Dental unit control

Control panel



Touch screen is unlocked. Press to lock.



Touch screen is locked. Press and hold to unlock.

Door open / assistant call function for preprogrammed time

Short activation



Door open / assistant call function as long as pressed

Long activation

Operating light On ► Off

Short activation



Intensity of operating light

Long activation

Operating light's composite mode On ► Off

Short activation



Intensity of operating light in composite mode

Long activation

Start required timer



→ Select timer number

Maintenance procedure



→ Select procedure

Foot control


No instrument activated

Short activation

Door open / assistant call function for preprogrammed time

Long activation

Door open / assistant call function as long as pressed

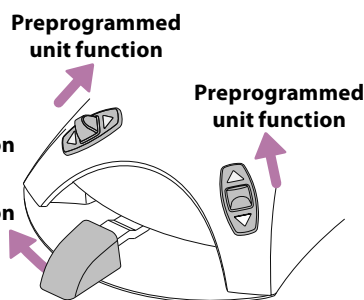

Instrument control

Control panel



Touch screen is unlocked. Press to lock.



Touch screen is locked. Press and hold to unlock.


<p>Micromotor or turbine Automatic chip blow On ► Off</p>	<p>Micromotor, turbine or scaler Instrument light On ► Off</p>	<p>Micromotor or turbine Water & air ► Air ► No spray Scaler Spray 1 ► Spray 2 ► No spray</p>
<p>Scaler Change operation mode</p>	<p>Turbine Power reduction On ► Off</p>	<p>Turbine Quickstart On ► Off</p>
<p>Micromotor Reverse rotation On ► Off</p>	<p>Micromotor RPM limit On ► Off</p>	<p>Micromotor Bien-Air MX2 Preset selection</p>
<p>Micromotors Bien-Air MX2 and Bien-Air MCX Torque limit On ► Off</p>	<p>Micromotor Bien-Air MX2 Toggle drive mode when torque limit On</p>	<p>Auto stop</p>
		<p>Auto reverse</p>

Foot control

Unit controlled instrument activated

Micromotor or turbine (standard pedal)

Drive instrument

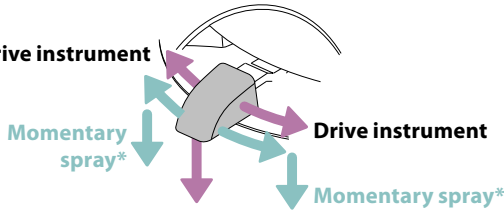

Short activation

Water & air ► Air ► No spray


Long activation

Manual chip blow

*If enabled by service technician

Scaler (standard pedal)

Drive scaler

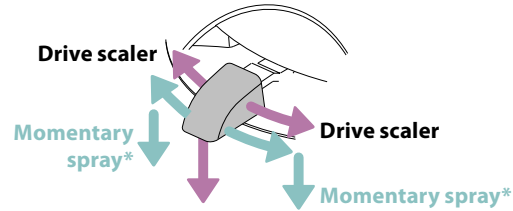


Short activation

Spray 1 ► Spray 2 ► No spray

*If enabled by service technician

Micromotor, turbine or scaler


Preprogrammed instrument function**

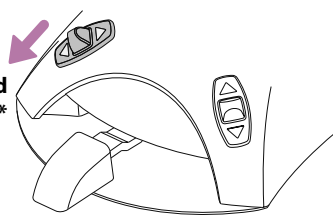

**Can be changed by service technician


Polymerisation light

Start ► Stop

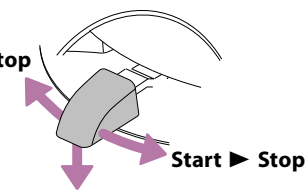

Start ► Stop

Intraoral camera

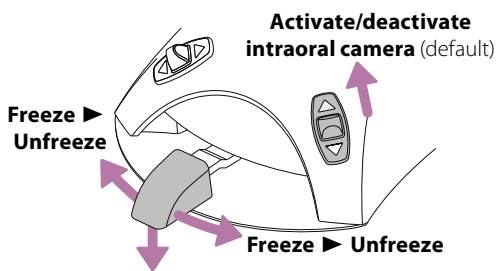


Short activation

Save still picture

Planmeca intraoral scanner

Activate/deactivate instrument view*

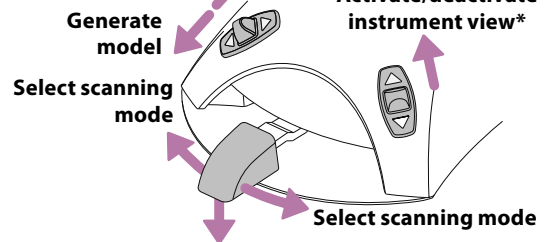

Short activation

Start scanning

Long activation

Take image

*If enabled by service technician

Programming

Control panel



Touch screen is unlocked. Press to lock.



Touch screen is locked. Press and hold to unlock.

Patient chair autoposition settings



The function is enabled.



The function is disabled.



Unit settings




The function is enabled.



The function is disabled.

Most programming follows this simple sequence:

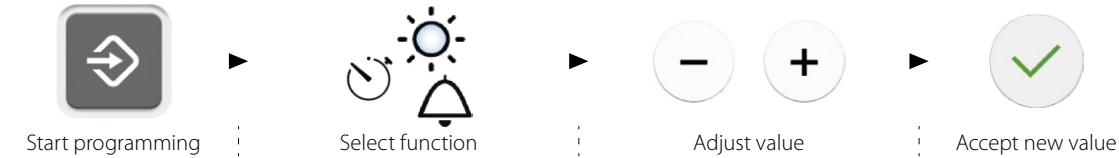

Instrument settings




The function is enabled.



The function is disabled.

Most programming follows this simple sequence:

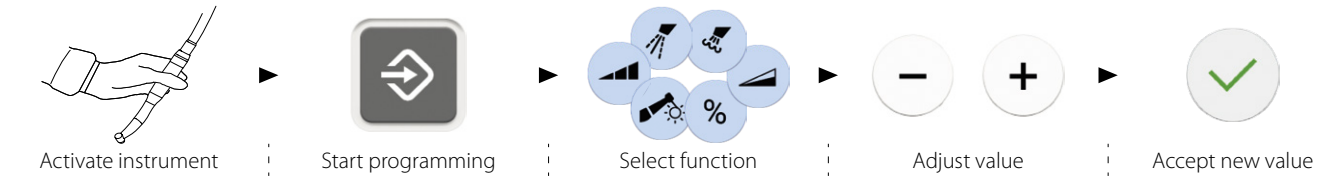

Time and date settings



The function is enabled.



The function is disabled.

